

Top of the Rion Range of Sound Level Meters

Sound level meter
and 1/3 octave band real-time analyzer

NA-28


Easy to use compact design with comprehensive features

Rion's priorities for on-site measurements are speed, ease of use, quality and reliability.

The New NA-28 is the top of the Rion range of sound level meters and analyzers. It combines cutting edge technology with excellent quality and unrivalled ease of use.

Key Features Include:


- Ease of use - main functions on dedicated, backlit keys
- Superb high-contrast backlit TFT-LCD color display
- Simultaneous measurement and display of 1/1 and 1/3 octaves
- One keystroke to switch between sound level meter and analyzer display
- Massive storage capacity using text files stored to CompactFlash memory cards (CF card)
- Flexible and simple PC connectivity (CF card and USB Virtual Disk)
- Exceptional battery life using standard alkaline batteries, approx. 16 hours

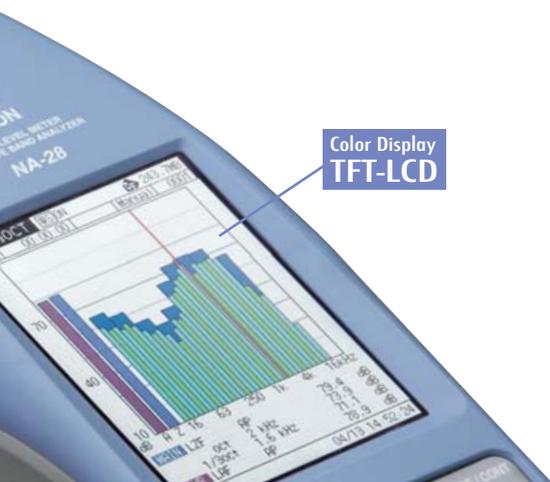

Sound level meter and 1/3 octave band real-time analyzer

NA-28

System constitution

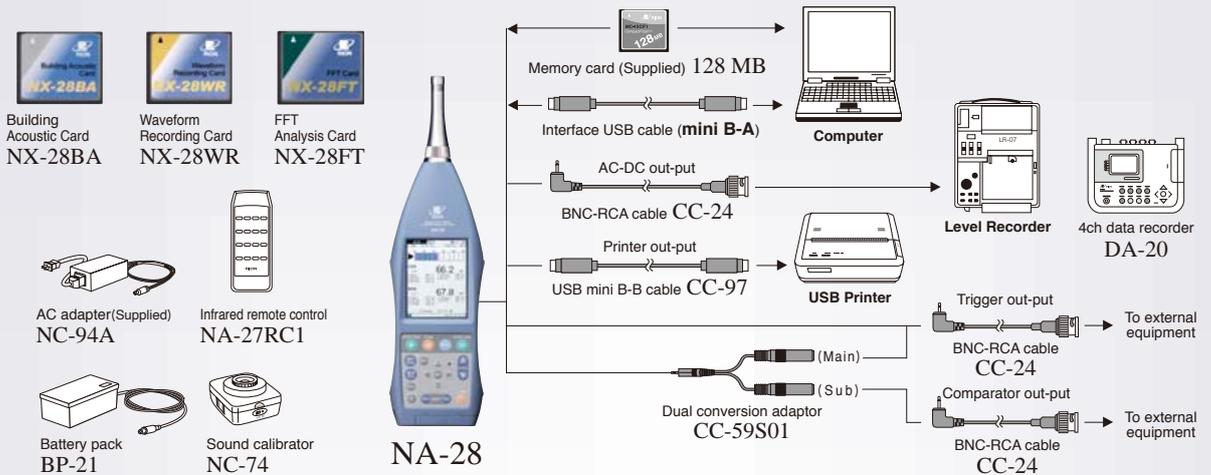

Key Capabilities

- Real Time Octaves (16 Hz to 16 kHz) or 1/3 octaves (12.5 Hz to 20 kHz)
- Real Time Simultaneous Octaves (16 Hz to 8 kHz) and 1/3 Octaves (12.5 Hz to 12.5 kHz)
- Data stored as text files direct to CF card
- Measures and logs L_{eq} , L_{max} , L_{min} and 5 percentile values (L_N) in octaves and/or 1/3 octaves
- Auto Stores 300 000 data sets or 1 000 hours of 1 second 1/3 octaves onto 1 GB CF card
- Auto Stores 1 000 data sets or 10 000 of 1 second 1/3 octaves to internal memory
- Manual Storage for 1 000 data sets internally or 100 000 data sets to 1 GB CF card
- Linearity 110 dB in Sound Level Meter Mode and 95 dB in Analyzer Mode
- 16 hours battery life with 4 Alkaline 'C' Cells
- Main and Sub-Channel for simultaneous selection of 2 time or frequency weightings
F (Fast), S (Slow), 10 ms Time Weightings plus Peak & Impulse on Sub-Channel
- Data transfer using CF card or USB (meter/CF card appearing as virtual disk)
- Measurement can be started by internal or external trigger
- Comparator output to trigger external devices
- AC and DC outputs of main and/or sub-channel
- Expandable functionality using programme cards

Key Options

- Building Acoustics Programme Card
- Uncompressed WAV file recording Programme Card


Flexible user interface

- 1 CF card slot
- 2 Infrared remote control sensor
- 3 AC adapter terminal
- 4 Two-way trigger input/comparator output terminal
- 5 AC output terminal
- 6 DC output terminal
- 7 USB terminal




[Terminals on lower surface]


Screen display-Example

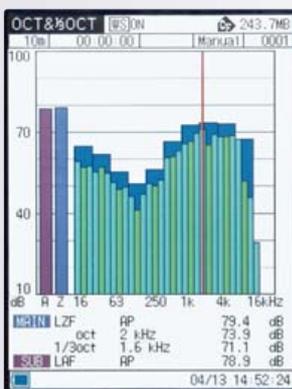


Analysis mode screen
(Simultaneous 1/1 & 1/3 octave band display)

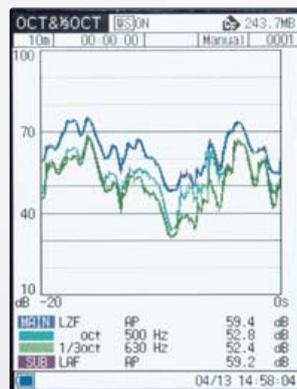

Time versus level display
with 1/1, 1/3 octave analysis

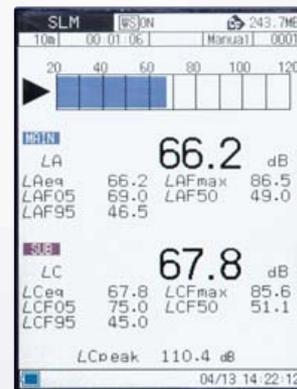

Sound level meter mode screen
(Sound level display)

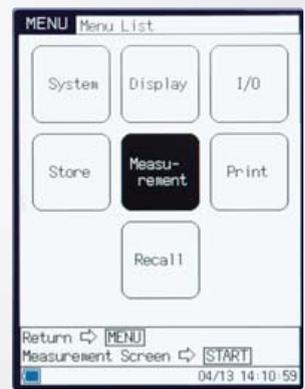

Menu list screen

USB Printer
BL-112UI OPTION



Infrared Remote Control
NA-27RC1 OPTION



Memory Card 128 MB
MC-12CF1 SUPPLIED





Waveform Recording Card NX-28WR

NX-28WR is a program card that provides the NA-28 with recording functions. Using the NA-28 and NX-28WR in combination makes it possible to measure sound pressure levels together with sound pressure waveforms during frequency analysis. Since the data are recorded in uncompressed WAVE files, they can be handled with software*1 compatible with the WAVE and analyzed.

*1 Software may not be compatible depending on sampling frequencies. If the software is not compatible, use a sampling converter to change sampling frequencies.

	128 MB	256 MB	1 GB	2 GB
48 kHz	15 m	30 m	2 h 10 m	4 h 40 m
24 kHz	30 m	1 h	4 h 20 m	9 h 20 m
12 kHz	1 h	2 h 10 m	8 h 50 m	18 h 50 m
64 kHz	10 m	20 m	1 h 40 m	3 h 30 m
32 kHz	20 m	50 m	3 h 20 m	7 h
16 kHz	50 m	1 h 40 m	6 h 40 m	14 h 10 m

Recording time would be somewhat changed by the number of files including recording data.

Feature 1 Replay of recorded sound – It is possible to immediately identify unnecessary or unknown sounds by listening to the recorded data*2

*2 Using Windows Media Player

- I conducted sound analysis but there are irregularities in the analysis results and I don't know what causes them.
- I detected the sound of a police car siren during measurement of traffic noise and I would like to exclude it.
- I measured sound levels and would like to listen to specific events.

Feature 2 Reanalysis of recorded sound – It is possible to reanalyze data based on the recorded waveforms using waveform analysis software

- I conducted 1/1 octave band analysis but I need to be able to conduct 1/3 octave band analysis.
- I conducted 1/3 octave band analysis but I need to be able to conduct analyses in more detail by FFT.

Specifications

Sampling frequency	Octave, 1/3 octave simultaneous analysis	48 kHz, 24 kHz, 12 kHz
Sound meter, octave analysis, 1/3 octave analysis		64 kHz, 32 kHz, 16 kHz
Quantization bit length		16 bit
Data format		WAVE
Frequency weighting		Z weighting (flat response) (fixed)
Recording functions		
Event mode		Level recording, interval recording, manual recording
Total mode		Total recording
Simultaneous use with Building Acoustics Card NX-28BA		
During sound insulation and impact sound measurement		Total recording
During reverberation time measurement		Total recording with pre-trigger (1 s)

Replay and reanalysis cannot be made with the NA-28 unit.

Software Recorded data by NX-28WR can be displayed and analyzed using optional software.

Optional accessory


Waveform processing software
DA-20PA1



Octave band analysis screen

Optional accessory

Waveform analysis software
CAT-WAVE

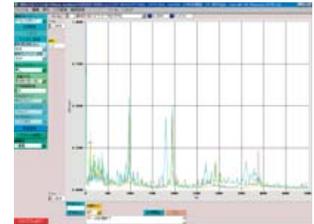

Spectrum map screen



NX-28FT program card adds FFT analysis capability to NA-28.


- Analysis frequency range: 20 kHz (fixed)
- Number of analysis lines: 8,000 (fixed) (frame time 400 ms, frequency resolution 2.5 Hz)

FFT Analysis Card NX-28FT


Specifications

Standard compliance	ISO 1996-2: 2007 Annex C *1
Measurement mode (FFT mode)	Main channel all-pass value and FFT analysis Sub-channel all-pass value
Measurement items	Simultaneous measurement of INST and LIN or MAX Measurement time 1 to 999 seconds
Dynamic range	100 dB
Analysis frequency range	20 kHz (fixed)
Time window functions	Hanning, Rectangular
Number of spectrum lines	8,000 (fixed) (frame time 400 ms, frequency resolution 2.5 Hz)
Sampling frequency	48 kHz (fixed)
Display	
Measurement screen	Simultaneous display of FFT analysis result and all-pass level
Number of FFT display lines	200
Zoom ratio	x1, x2, x5, x10, x20, x40
Top list screen	List display of frequency and level values for top 20 lines, in descending order
Trigger	Controls start of measurement and memory store operation
Level trigger	Measurement starts when threshold level (selectable in 1 dB steps) is exceeded, and ends after preset measurement time has elapsed. Trigger source: main channel all-pass value only. Slope fixed to +.
External trigger	Measurement starts at falling edge of logic level signal supplied to trigger input.
Store function	
Manual store	Stores measurement results.
Number of data sets	
CF card*2	Max. 20 store names, with up to 100 data sets each (Store to internal memory not supported)
Combination with NX-28WR	Allows waveform recording under measurements for LIN, MAX. Waveform data stored together with manual store data on CF card.

*1 Only frequency analysis is performed on unit. Tonal index calculation is performed on computer.
*2 Use only RION supplied cards for assured operation.

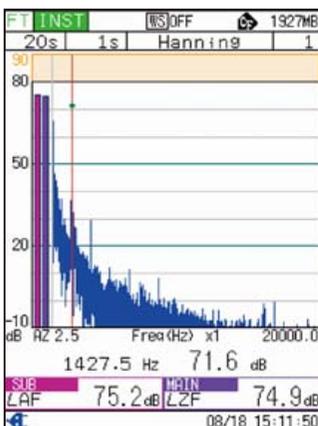

Measurement screen (zoom factor x1)

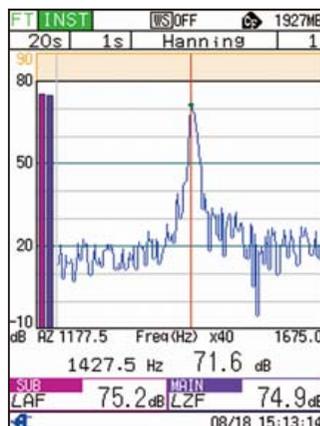

Measurement screen (zoom factor x40)



Building Acoustic Card NX-28BA

NX-28BA is a program card used in NA-28 for simple and easy measurement of airborne and floor impact sound insulation of buildings and the reverberation time. The measurements conforming to ISO and single-number quantities can also be calculated by the main body of NA-28. Data is stored as text files. Furthermore, when used in conjunction with the waveform recording card NX-28WR, sound waveforms during measurement can be recorded simultaneously.

Applicable specifications


- ISO 140-4 Acoustics – Measurement of sound insulation in buildings and of building elements – Part 4: Field measurements of airborne sound insulation between rooms
- ISO 140-7 Acoustics – Measurement of sound insulation in buildings and of building elements – Part 7: Field measurements of impact sound insulation of floors
- ISO 717-1 Acoustics – Rating of sound insulation in buildings and of building elements – Part 1: Airborne sound insulation
- ISO 717-2 Acoustics – Rating of sound insulation in buildings and of building elements – Part 2: Impact sound insulation
- ISO 140-5* Acoustics – Measurement of sound insulation in buildings and of building elements – Part 5: Field measurements of airborne sound insulation of façade elements and façades
- ISO 16032* Acoustics – Measurement of sound pressure level from service equipment in buildings – Engineering method

*The main body performs measurement only.

Screen display – Example

MENU Building Acoustic	
Measurement Mode	AirRm(D)
Store Name	DD_0001
Measurement Time	10s
Source Position	2
Source Room Meas. Pos.	5
Receive Room Setting	
Measurement Position	5
BGN Mode	Before
Source Room Data	None
Surface Area	172.0m ²
Room Volume	043.0m ³
Return	MENU
Measurement Screen	START

Setup menu of airborne sound insulation measurement between two rooms

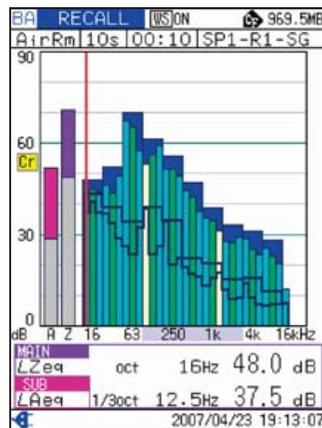

Measurement results overlaid with background noise (for octave, 1/3 octave simultaneous analysis)

BA RECALL [US]OFF 1921MB	
AirRm 10s 00:10 S.N.Q	
R' _w	40 dB
D _{n,w}	33 dB
D _{nT,w}	39 dB
C	0 dB
C _{tr}	-2 dB
D _{nT,A,k}	40 dB
I _{lu,k}	-12 dB


Single-number quantities of airborne sound insulation between rooms

BA RECALL [US]ON 1921MB	
Imp-L 10s 00:00 S.N.Q	
L' _{n,w}	61 dB
L' _{nT,w}	60 dB
L' _{nT,A}	58 dB
CI	-2 dB
I _{co}	1 dB

Single-number quantities of floor impact sound insulation (light impact source)


BA RECALL [US]ON 1734MB					
RT_0100_04 Print MODE					
Freq. (oct)	T20	T30	Txx	Error (°)	
16	0.58	0.77	---	33	
31.5	1.25	---	E1	---	
63	0.95	1.03	0.99	8	
125	0.50	0.89	0.74	78	
250	0.64	0.60	0.60	6	
500	0.61	0.60	---	2	
1k	0.47	0.44	0.45	6	
2k	0.48	0.44	0.45	8	
4k	0.42	0.43	---	2	
8k	0.38	0.41	---	8	

Measured value list of reverberation time

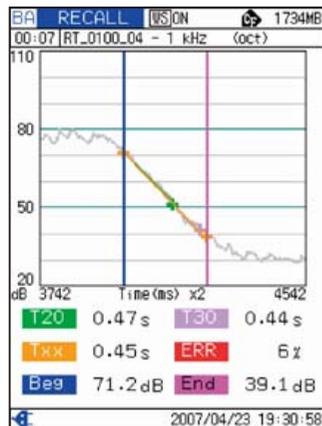

Measurement results of reverberation time decay curve

Measurement of reverberation decay curve

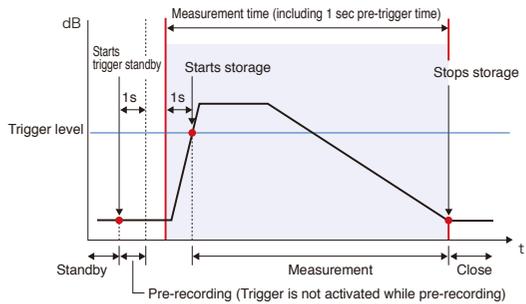

Specifications

Analysis mode	Real-time octave band analysis, Real-time 1/3 octave band analysis Real-time octave, 1/3 octave band simultaneous analysis (Sound level meter mode is not available)
Measurement items (vary with measurement mode)	Instantaneous sound pressure level L_p Equivalent continuous sound pressure level L_{eq} Maximum instantaneous sound pressure level L_{max}
Measurement of airborne sound insulation between two rooms	
Settings	Measurement time 1 to 60 sec Number of setting sound sources 1 to 8 points Number of measurement points in sound source room 1 to 10 points Number of measurement points in sound receptor room 1 to 10 points Background noise measurement mode None (none)/Once (1 point)/Before/During
Calculations	Average measured value, single number quantity, insulation factor value (D-value)
Display	L_p/L_{eq} (Background noise sound level), $L_p/L_{eq}/L_{max}$ (Sound level in sound receiving room) Displays results overlaid with background noise (for measurement in sound receiving room) Displays alarm when the SPL difference with background noise is too small (for measurement in sound receiving room)
Measurement of floor impact sound insulation (for light impact source)	
Settings	Measurement time 1 to 60 sec Number of setting sound sources 1 to 8 points Number of measurement points in sound receiving room 1 to 10 points Background noise measurement mode None (none)/Once (1 point)/Before/During
Calculations	Average measured value, single number quantity, insulation factor value (LL-value)
Display	L_p/L_{eq} (Background noise sound level), $L_p/L_{eq}/L_{max}$ (Sound pressure level in sound receiving room) Displays results overlaid with rating curve Displays results overlaid with background noise Displays alarm when the SPL difference with background noise is too small
Measurement of floor impact sound insulation (for heavy impact source)	
Settings	Measurement time 1 to 60 sec Number of setting sound sources 1 to 8 points Number of measurement points in sound receiving room 1 to 10 points Number of measurements 1 to 5 times Background noise measurement mode None (none)/Once (1 point)/Before/During
Calculations	Insulation factor value (LH-value)
Display	L_p/L_{eq} (Background noise sound level), L_p/L_{max} (Sound pressure level in sound receiving room) Displays results overlaid with rating curve Displays results overlaid with background noise Displays alarm when the SPL difference with background noise is too small
Measurement of indoor noise rating	
Calculations	Indoor noise rating value (NC-value or N-value)
Display	Displays results overlaid with rating curve
Measurement of reverberation time	
Settings	Interrupted noise method Measurement time 2 to 60 sec (varies with sampling cycle) Repeat count 1 to 10 times
Calculations	T20, T30 (using the least squares method) Reverberation time calculated for random segments
Display	Averaged reverberation time, reverberation decay curve
Other measurements	Measurement of exterior wall sound insulation, Measurement of equipment noise
Other capabilities	Dedicated address display and Auto-increment, Alarm display, Settings change monitoring function, Waveform recording function (NX-28WR is separately needed)

Specifications

Applicable specifications	Sound level meter: Measurement method precision sound level meter IEC 61672-1: 2002 Class 1 IEC 61260 : 1995 Class 1 ANSI S1.4-1983 Type 1 ANSI S1.43-1997 Type 1 ANSI S1.11-2004 Class 1 JIS C 1509-1: 2005 Class 1 JIS C 1513 : 2002 Class 1 JIS C 1514 : 2002 Class 1				
Measurement functions	With both a sound level meter mode and analyzer mode, it is capable of simultaneous main channel and sub-channel measurement in either mode. Time and frequency weighting are set separately for the main and sub-channels.				
Measurement modes	<table border="1"> <tr> <td>Sound level meter mode</td> <td>Measurement of all-pass values indicated in the measurement items below in the main or sub-channel Measurement of either L_{peak} or L_{rms} in the sub-channel</td> </tr> <tr> <td>Analyzer mode</td> <td>Real-time octave and 1/3 octave band analysis and all-pass measurement in the main channel Only all-pass measurement in the sub-channel</td> </tr> </table>	Sound level meter mode	Measurement of all-pass values indicated in the measurement items below in the main or sub-channel Measurement of either L_{peak} or L_{rms} in the sub-channel	Analyzer mode	Real-time octave and 1/3 octave band analysis and all-pass measurement in the main channel Only all-pass measurement in the sub-channel
Sound level meter mode	Measurement of all-pass values indicated in the measurement items below in the main or sub-channel Measurement of either L_{peak} or L_{rms} in the sub-channel				
Analyzer mode	Real-time octave and 1/3 octave band analysis and all-pass measurement in the main channel Only all-pass measurement in the sub-channel				
Measurement items	Simultaneous measurement of all items in the selected time weighting and frequency weighting characteristics 1) Instantaneous sound pressure level L_p 2) Equivalent continuous sound pressure level L_{eq} 3) Sound exposure level L_E 4) Maximum sound pressure level L_{max} APMax and BandMax can be selected as maximum 5) Minimum sound pressure level L_{min} 6) Maximum 5 time ratio sound levels L_N (1 to 99 %, 1 % Step) Calculation from L_p or $L_{eq,1sec}$ One of the following is possible in the sub-channel in the sound level meter mode: Peak sound level L_{peak} Takt-max sound pressure level L_{rms} Frequency weighting characteristics are the same as sub-channel				
Measurement time	1 to 59 sec, 1 to 59 min, 1 to 24 hours				
Microphone and preamplifier	Microphone: UC-59 Sensitivity: -27 dB±2 dB (re 1 V/Pa) Preamplifier: NH-23				
Measurement range	A 25 dB to 130 dB C 33 dB to 130 dB Z 38 dB to 130 dB				
Total range (A-characteristics, 1 kHz)	25 dB to 140 dB				
Maximum peak sound level measurement	143 dB				
Inherent noise	A 17 dB or less C 25 dB or less Z 30 dB or less				
Frequency range	10 Hz to 20 kHz				
Analysis frequency range	Center frequency Octave analysis 16 Hz to 16 kHz (simultaneous analysis : up to 8 kHz) 1/3 octave analysis 12.5 Hz to 20 kHz (simultaneous analysis : up to 12.5 kHz)				
Frequency weighting	A, C and Z				
Time weighting	Main channel F (Fast), S (Slow), 10 ms Sub-channel F (Fast), S (Slow), 10 ms, Impulse				
Linear operating range	All-pass (A-characteristics) 110 dB Spectrum 95 dB				
Level range	Sound level meter mode Bar graph display range: maximum 100 dB 30 dB to 130 dB 20 dB to 120 dB 20 dB to 110 dB 20 dB to 100 dB 20 dB to 90 dB 20 dB to 80 dB Analyzer mode Bar graph display range: 90 dB 40 dB to 130 dB 30 dB to 120 dB 20 dB to 110 dB 10 dB to 100 dB 0 dB to 90 dB -10 dB to 80 dB				
Sampling frequency	L_{eq} , L_E , L_{max} , L_{min} , L_{peak} 15.6 μ s (20.8 μ s for octave, 1/3 octave simultaneous analysis) L_N 100 ms				
Correction functions	Windscreen correction Frequency response correction to ensure standard compliance with windscreen installed correction on/off setting via menu Diffuse sound field correction Correction of frequency characteristics in order to comply with standards (ANSI S1.4) in diffuse sound fields Correction function on/off operation implemented on the menu screen				
Display	Color semi-transparent TFT-LCD display with backlight (240 x 320 dots) Refresh cycle 100 ms				
Trigger	Controls measurement and memory storage start. Level 1 Measurement starts with the trigger level (1 dB intervals) as threshold and stops when the set measurement times elapses. Slope +/- is set. Level 2 1 time only measurement when the trigger level is exceeded. External Starts when a falling signal in the logic level of the external trigger terminal is detected. Time Sets start time and trigger repeat interval.				
Delay time	After the start key is pressed, the time until the start of the measurement or trigger detection is set. Time setting 1 sec intervals within the range of 0 to 10 sec				
Back erase function	Measurement is temporarily suspended by pressing the pause key and the previous 5 seconds of data is eliminated from the calculation.				
Storage	The sound level or calculation results are recorded in the manual or auto-store mode. Data is recorded either in the internal memory or CF card. Internal memory has 1 block and it is possible to select either manual storage or auto-storage 1, 2.				

* Specifications subject to change without notice.

Distributed by:

Manual store	Manual recording of measurement results per address together with the measurement start time																												
Record data count	<table border="1"> <tr> <td>Internal memory</td> <td>Maximum 1 000 sets</td> </tr> <tr> <td>CF card*</td> <td>Maximum 1 000 sets per store name, maximum 100 store names can be stored</td> </tr> </table>	Internal memory	Maximum 1 000 sets	CF card*	Maximum 1 000 sets per store name, maximum 100 store names can be stored																								
Internal memory	Maximum 1 000 sets																												
CF card*	Maximum 1 000 sets per store name, maximum 100 store names can be stored																												
Auto store	Continuous recording of measurement results at the set time interval (It is possible to append 4 types of marker data in order to be able to identify events that occur while recording) Pause does not function during auto-storage																												
Auto 1	<table border="1"> <tr> <td>Measurement time</td> <td>Maximum time: 1 000 hours (when using the CF card, refer to the following if using internal memory)</td> </tr> <tr> <td>Sound level meter mode</td> <td>Continuous recording in the CF card every 100 ms of L_p, L_{eq}, L_{max} and L_{min} as 1 set It is not possible to record sub-channel measurement results.</td> </tr> <tr> <td>Sampling cycle when using internal memory</td> <td>100 ms (L_p, L_{eq}, L_{max}, L_{min}) only Maximum time: 3 hours</td> </tr> <tr> <td>Analyzer mode</td> <td>Continuous recording in CF card instantaneous sound pressure level (L_p) in each band level and all-pass values</td> </tr> <tr> <td>Main channel</td> <td>All-pass values and band level values</td> </tr> <tr> <td>Sub-channel</td> <td>All-pass values only</td> </tr> <tr> <td>Sampling cycle when using internal memory</td> <td>1 ms to 1 sec, $L_{eq,1s}$ Maximum 10 000 sets (1 sec or, for $L_{eq,1s}$, 2.7 hours)</td> </tr> </table>	Measurement time	Maximum time: 1 000 hours (when using the CF card, refer to the following if using internal memory)	Sound level meter mode	Continuous recording in the CF card every 100 ms of L_p , L_{eq} , L_{max} and L_{min} as 1 set It is not possible to record sub-channel measurement results.	Sampling cycle when using internal memory	100 ms (L_p , L_{eq} , L_{max} , L_{min}) only Maximum time: 3 hours	Analyzer mode	Continuous recording in CF card instantaneous sound pressure level (L_p) in each band level and all-pass values	Main channel	All-pass values and band level values	Sub-channel	All-pass values only	Sampling cycle when using internal memory	1 ms to 1 sec, $L_{eq,1s}$ Maximum 10 000 sets (1 sec or, for $L_{eq,1s}$, 2.7 hours)														
Measurement time	Maximum time: 1 000 hours (when using the CF card, refer to the following if using internal memory)																												
Sound level meter mode	Continuous recording in the CF card every 100 ms of L_p , L_{eq} , L_{max} and L_{min} as 1 set It is not possible to record sub-channel measurement results.																												
Sampling cycle when using internal memory	100 ms (L_p , L_{eq} , L_{max} , L_{min}) only Maximum time: 3 hours																												
Analyzer mode	Continuous recording in CF card instantaneous sound pressure level (L_p) in each band level and all-pass values																												
Main channel	All-pass values and band level values																												
Sub-channel	All-pass values only																												
Sampling cycle when using internal memory	1 ms to 1 sec, $L_{eq,1s}$ Maximum 10 000 sets (1 sec or, for $L_{eq,1s}$, 2.7 hours)																												
Auto 2	<table border="1"> <tr> <td>Sound level meter mode</td> <td>Continuous recording in CF card of main channel and sub-channel all-pass values and measurement start time for each measurement time</td> </tr> <tr> <td>Analyzer mode</td> <td>Continuous recording in CF card of main channel band levels and all-pass values and sub-channel all-pass values and measurement start time for each measurement time</td> </tr> <tr> <td>Record data count</td> <td>Internal memory: Maximum 1 000 sets CF card: Maximum 300 000 sets</td> </tr> </table>	Sound level meter mode	Continuous recording in CF card of main channel and sub-channel all-pass values and measurement start time for each measurement time	Analyzer mode	Continuous recording in CF card of main channel band levels and all-pass values and sub-channel all-pass values and measurement start time for each measurement time	Record data count	Internal memory: Maximum 1 000 sets CF card: Maximum 300 000 sets																						
Sound level meter mode	Continuous recording in CF card of main channel and sub-channel all-pass values and measurement start time for each measurement time																												
Analyzer mode	Continuous recording in CF card of main channel band levels and all-pass values and sub-channel all-pass values and measurement start time for each measurement time																												
Record data count	Internal memory: Maximum 1 000 sets CF card: Maximum 300 000 sets																												
Data recall	Stored data access and time/level display (selected frequency band 1 only)																												
Memory store of settings	Maximum 5 sets of settings can be stored in internal memory and retrieved Start-up is possible under file setting conditions stored in the CF card in advance.																												
Printout	Measurement results can be printed using the special USB printer(Optional)																												
Screen print mode	1-page printing of the displayed screen																												
Memory print mode	Continuous printing of data in the specified address range in memory																												
Input/output	<table border="1"> <tr> <td>AC output</td> <td>Selection and output of all-pass signals of either the main channel or sub-channel</td> </tr> <tr> <td>Output voltage</td> <td>1 V (effective value) at range full scale</td> </tr> <tr> <td>Output resistance</td> <td>600 Ω</td> </tr> <tr> <td>Load resistance</td> <td>10 kΩ or more</td> </tr> <tr> <td>DC output</td> <td>Selection and output of all-pass signals of either the main channel or sub-channel</td> </tr> <tr> <td>Output voltage</td> <td>3.0 V, 25 mV/dB at range full scale</td> </tr> <tr> <td>Output resistance</td> <td>50 Ω</td> </tr> <tr> <td>Load resistance</td> <td>10 kΩ or more</td> </tr> <tr> <td>Comparator output</td> <td>Open collector output. Determination is also possible at the band level. The terminal is also used for the external trigger.</td> </tr> <tr> <td>Maximum applied voltage</td> <td>24 V</td> </tr> <tr> <td>Maximum driving current</td> <td>50 mA</td> </tr> <tr> <td>External trigger input</td> <td>Falling edge is detected at 0V to 5 V logic level. The terminal is also used for the comparator.</td> </tr> <tr> <td>USB</td> <td>Besides connection to a PC as a storage device, it is also possible to use communication device class and execute control by communication commands (however, settings relating to the transfer of stored data and storage action are not possible with communication commands).</td> </tr> <tr> <td>Remote control reception</td> <td>Control of NA-28 by infrared remote control (remote control NA-27RC1, optional)</td> </tr> </table>	AC output	Selection and output of all-pass signals of either the main channel or sub-channel	Output voltage	1 V (effective value) at range full scale	Output resistance	600 Ω	Load resistance	10 k Ω or more	DC output	Selection and output of all-pass signals of either the main channel or sub-channel	Output voltage	3.0 V, 25 mV/dB at range full scale	Output resistance	50 Ω	Load resistance	10 k Ω or more	Comparator output	Open collector output. Determination is also possible at the band level. The terminal is also used for the external trigger.	Maximum applied voltage	24 V	Maximum driving current	50 mA	External trigger input	Falling edge is detected at 0V to 5 V logic level. The terminal is also used for the comparator.	USB	Besides connection to a PC as a storage device, it is also possible to use communication device class and execute control by communication commands (however, settings relating to the transfer of stored data and storage action are not possible with communication commands).	Remote control reception	Control of NA-28 by infrared remote control (remote control NA-27RC1, optional)
AC output	Selection and output of all-pass signals of either the main channel or sub-channel																												
Output voltage	1 V (effective value) at range full scale																												
Output resistance	600 Ω																												
Load resistance	10 k Ω or more																												
DC output	Selection and output of all-pass signals of either the main channel or sub-channel																												
Output voltage	3.0 V, 25 mV/dB at range full scale																												
Output resistance	50 Ω																												
Load resistance	10 k Ω or more																												
Comparator output	Open collector output. Determination is also possible at the band level. The terminal is also used for the external trigger.																												
Maximum applied voltage	24 V																												
Maximum driving current	50 mA																												
External trigger input	Falling edge is detected at 0V to 5 V logic level. The terminal is also used for the comparator.																												
USB	Besides connection to a PC as a storage device, it is also possible to use communication device class and execute control by communication commands (however, settings relating to the transfer of stored data and storage action are not possible with communication commands).																												
Remote control reception	Control of NA-28 by infrared remote control (remote control NA-27RC1, optional)																												
Power supply	Four IEC R14P (size"C") batteries or external power supply																												
Operating time (23 °C, normal operating conditions)	When following not functioning ; sub-channel, backlight, AC output, DC output, USB function, remote-control, autostore																												
Manganese batteries	R14PU, 6 hours																												
Alkaline batteries	LR14, 16 hours (10 hours if backlight is continuously activated)																												
AC adapter	NC-94A																												
External power supply voltage	5 V to 6 V (rated voltage: 6 V)																												
Consumption current	230 mA (during normal operation at rated voltage)																												
Ambient conditions for operation	-10 °C to +50 °C, 10 %RH to 90 %RH																												
Dimensions, weight	331 (H) x 89 (W) x 51 (D) mm, approx. 730 g (including batteries)																												
Supplied accessories	Memory card (128 MB) MC-12CF1 x 1, Storage case x 1, Soft case x 1, AC adapter NC-94A x 1, Windscreen WS-10 x 1, BNC-RCA cable CC-24 x 1, Strap x 1, IEC R14P (size"C") batteries (alkaline) x 4																												

Options

name	model	name	model
Building acoustic card	NX-28BA	Printer paper(10 rolls/pkg)	P-112-30
Waveform recording card	NX-28WR	USB miniB-B cable(For printer)	CC-97
FFT analysis card	NX-28FT	Battery pack	BP-21
Remote control	NA-27RC1	Dual output adaptor	CC-59S01
Sound calibrator	NC-74		
Memory card	128 MB, 256 MB, 1GB, 2 GB		
USB printer	BL-112UI		

* Use only RION supplied cards for assured operation.

ISO 14001 RION CO., LTD.
ISO 9001 RION CO., LTD.



RION CO., LTD.
http://www.rion.co.jp/english/

3-20-41, Higashimotomachi, Kokubunji, Tokyo 185-8533, Japan
Tel: +81-42-359-7888 Fax: +81-42-359-7442